

Fig. 1 – Prior art
Principle of reinjection in post-dilution

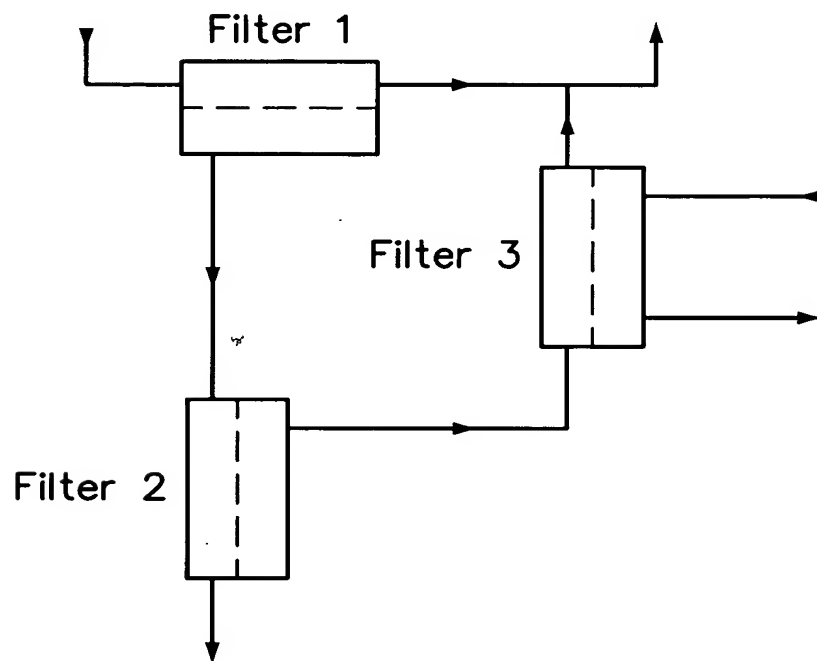


Fig. 2 – Prior art
Principle of reinjection in post-dilution

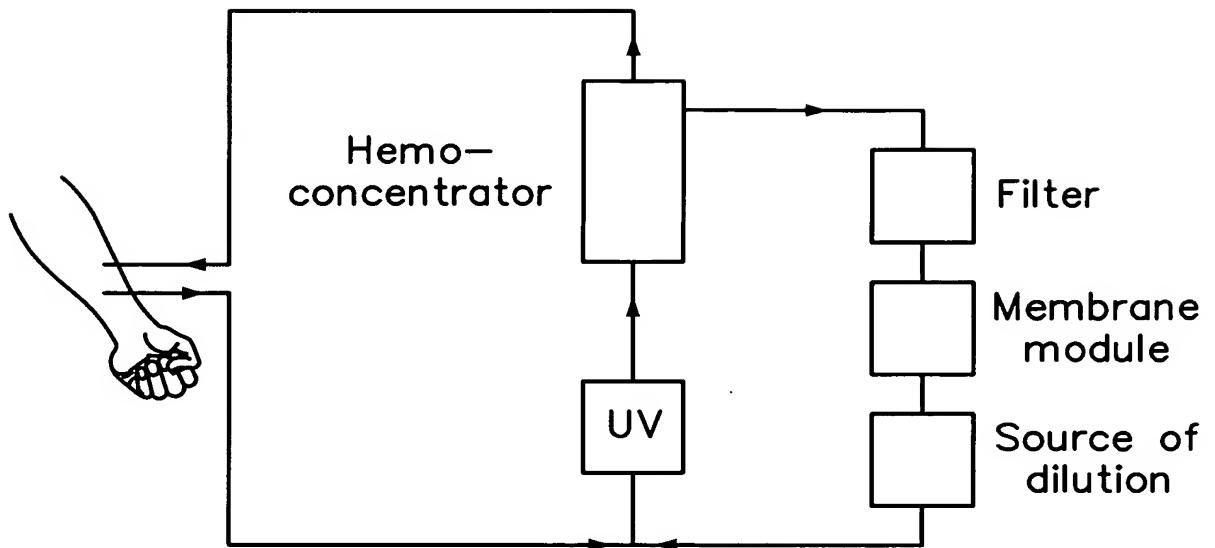


Fig 3. — Prior art

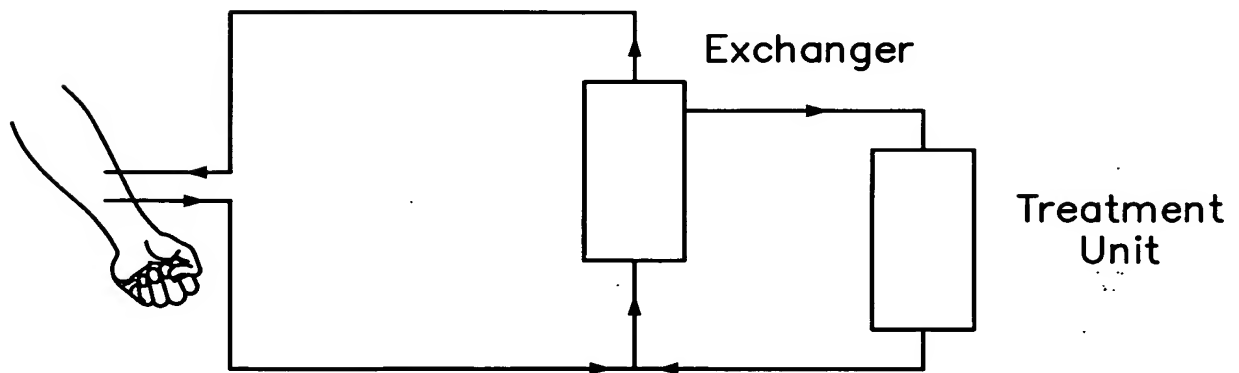


Fig. 4 — Principle of the invention

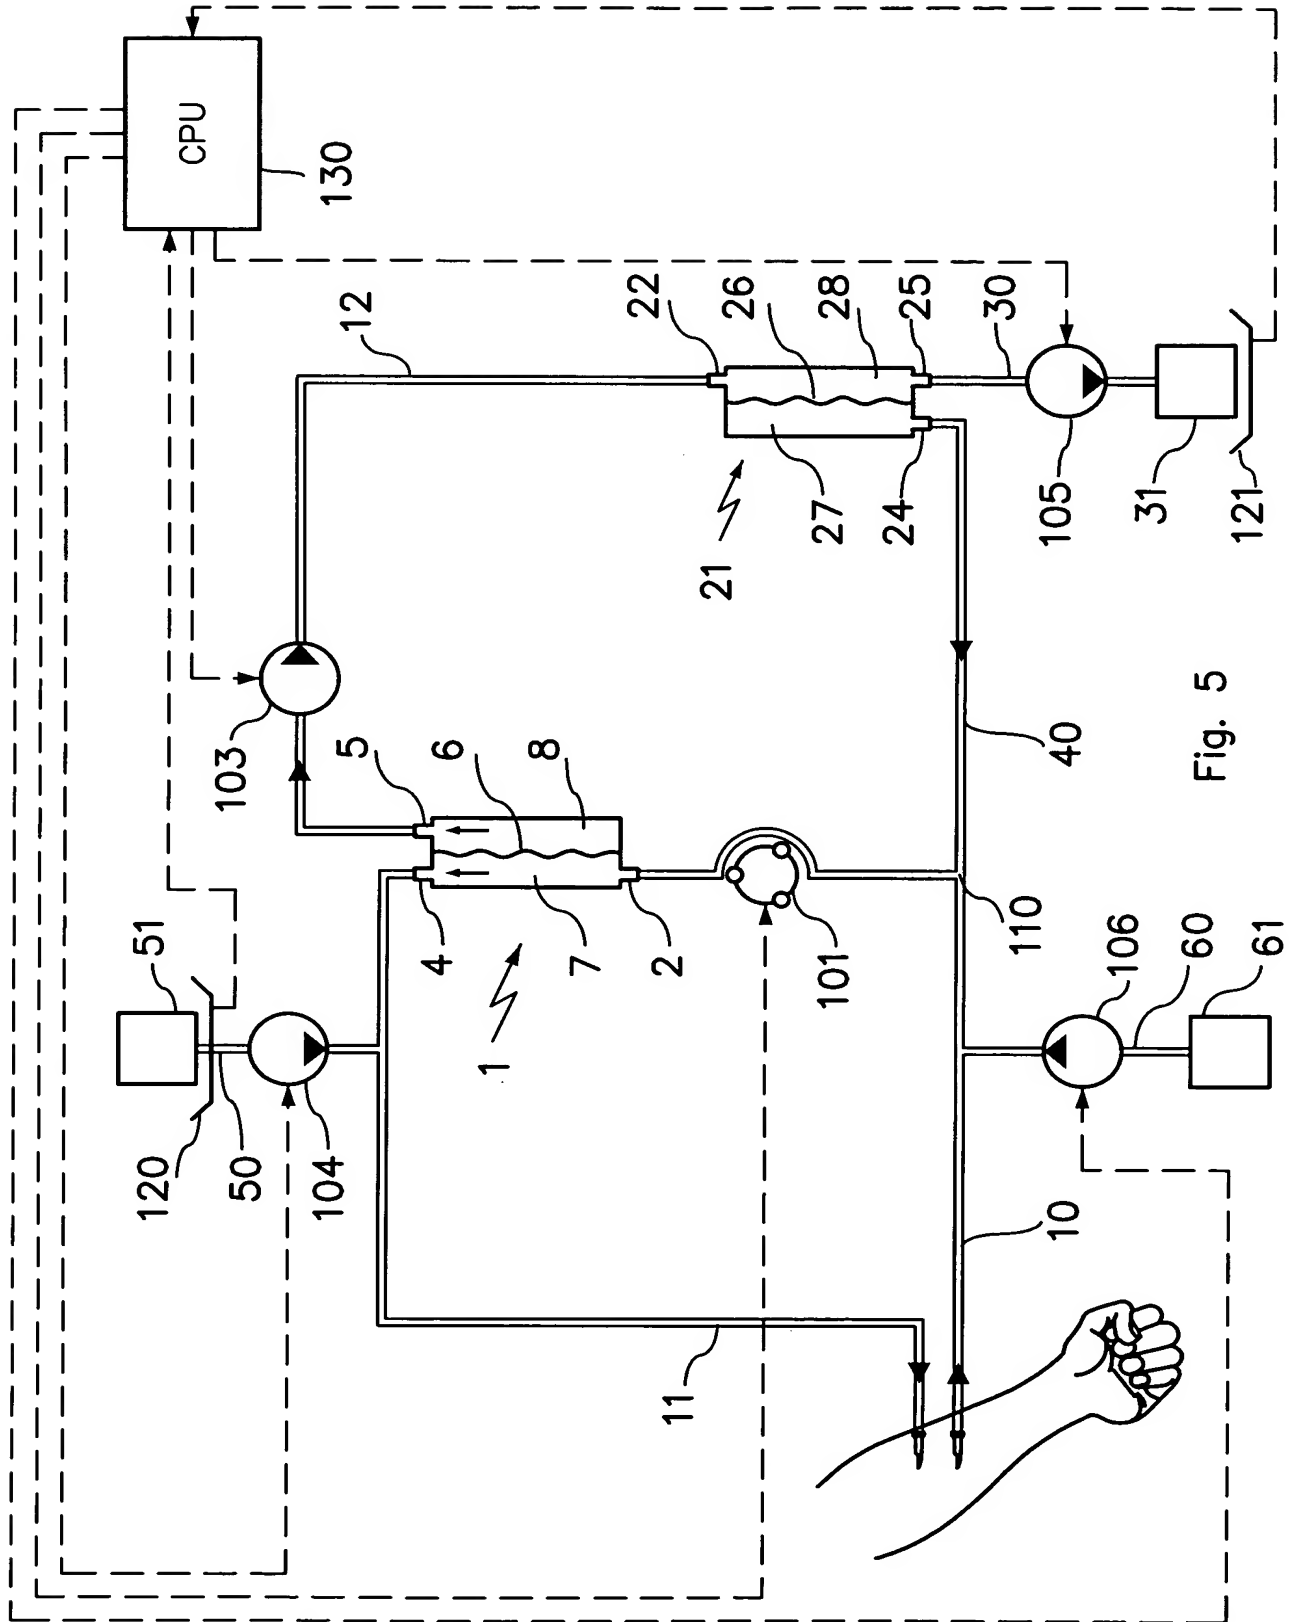




Fig. 6 – Exchanger in dialysis mode

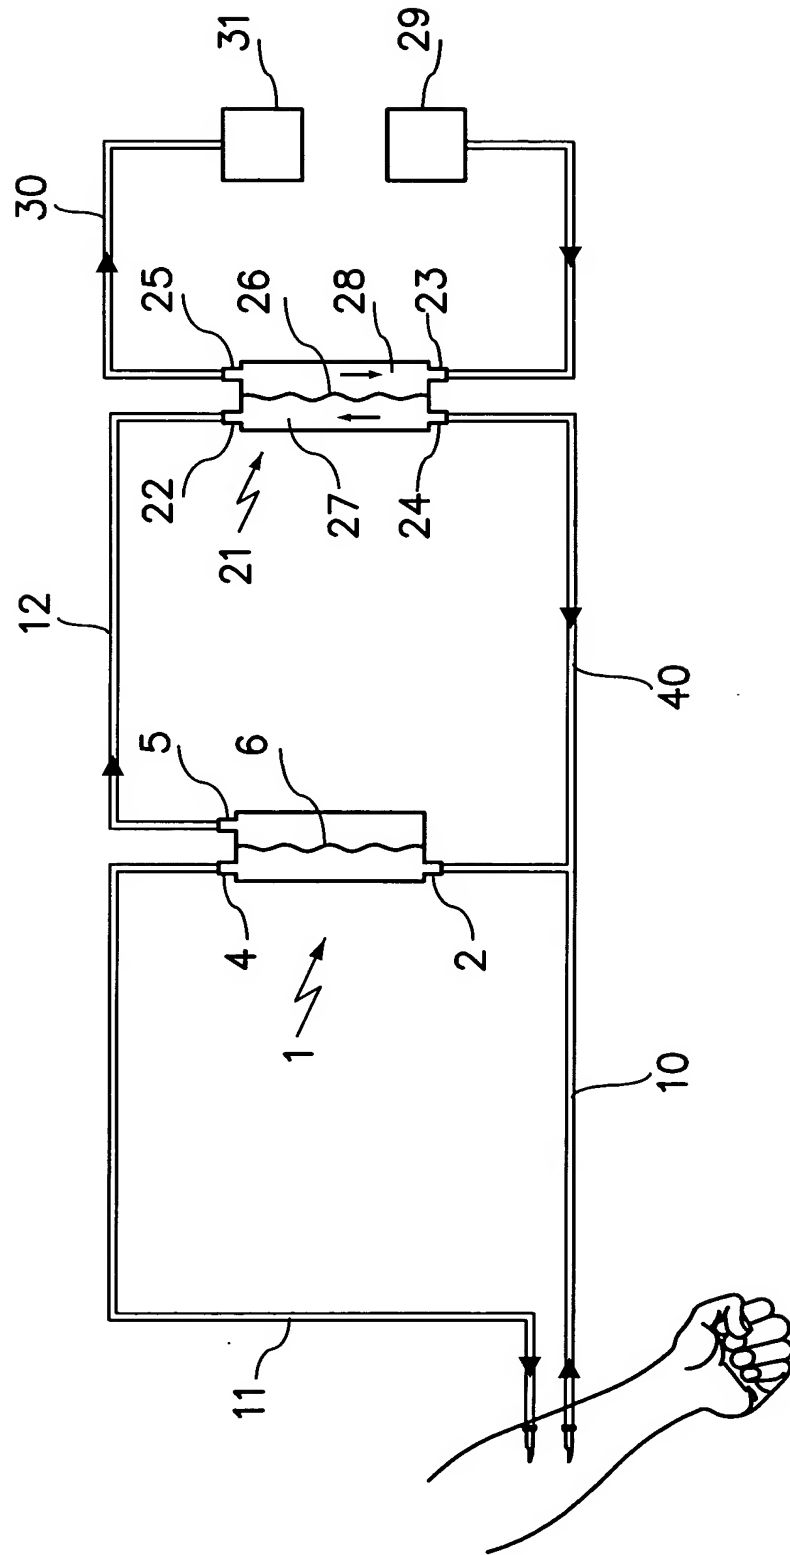


Fig. 7 – Treatment unit in dialysis mode



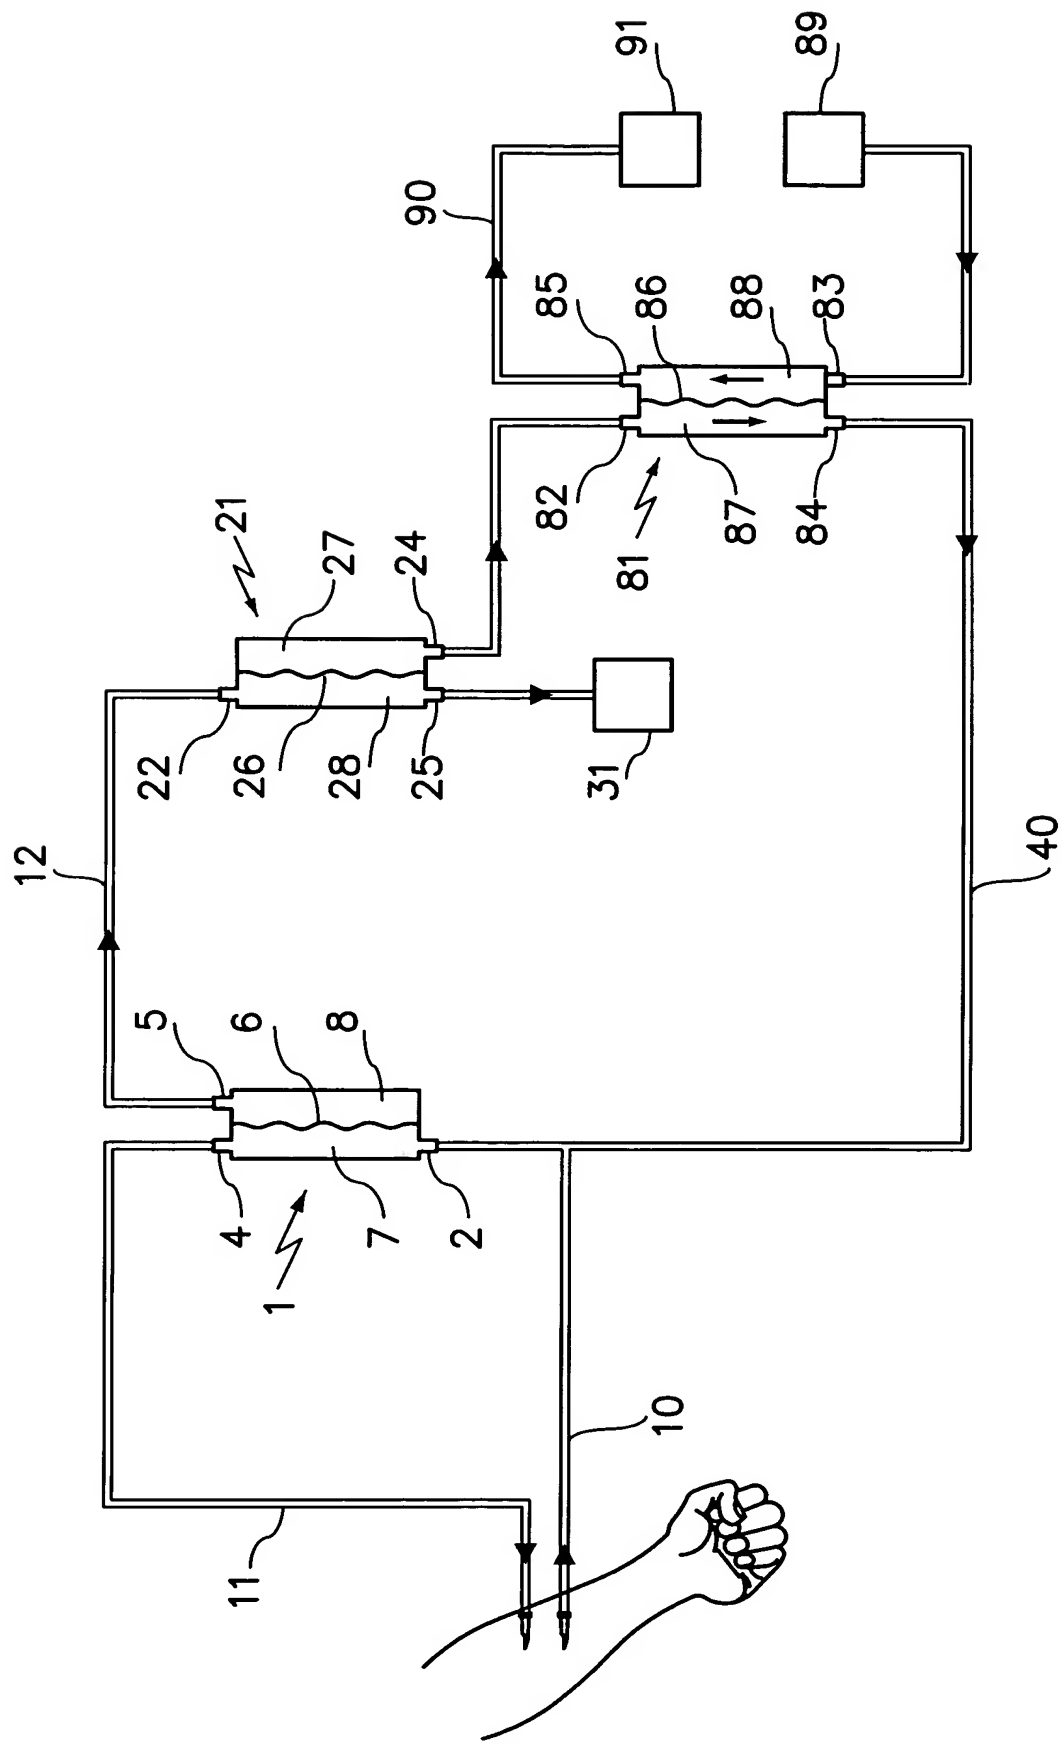


Fig. 8 – Auxiliary exchanger
in dialysis mode

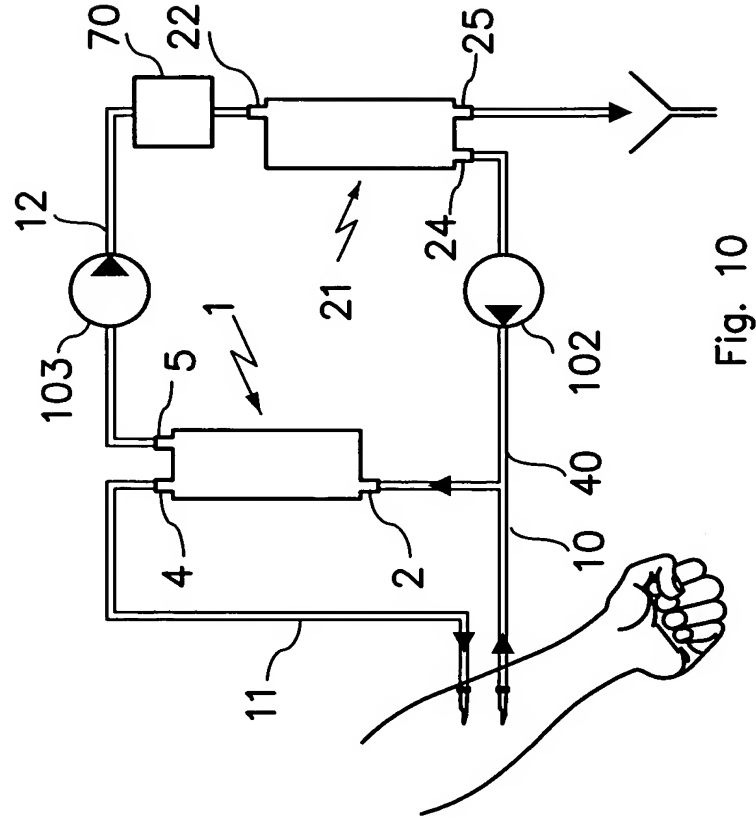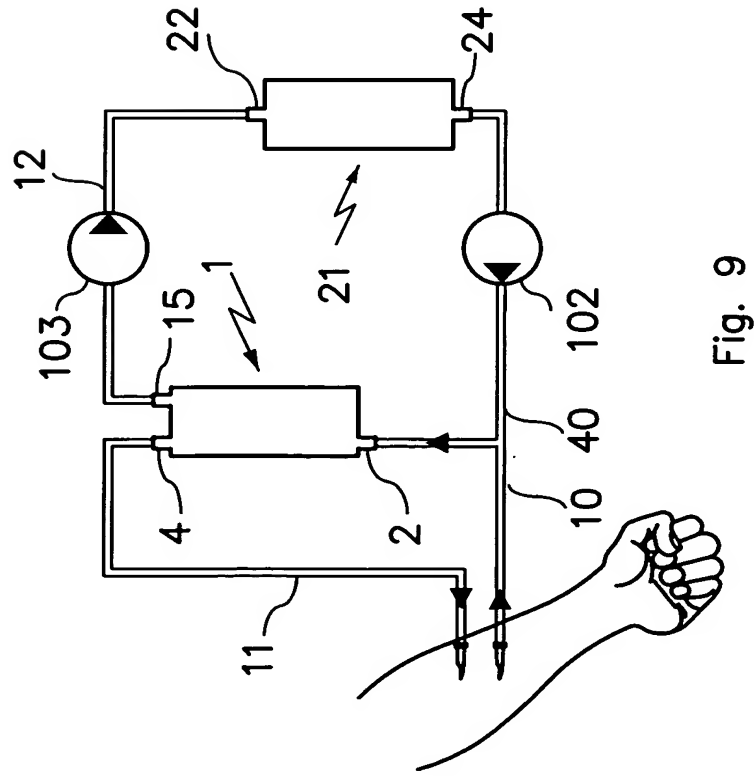

Plasmapheresis

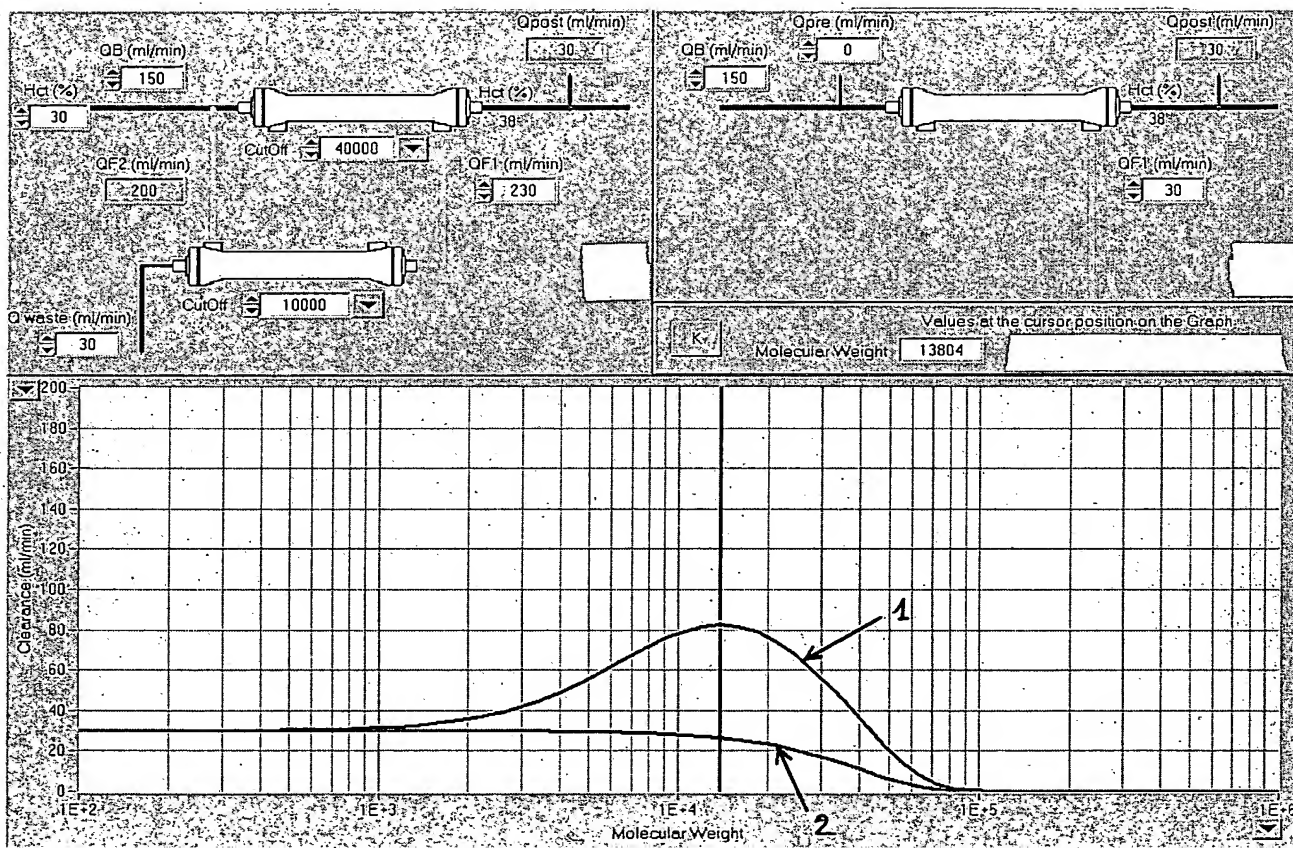


Fig. 11

BEST AVAILABLE COPY

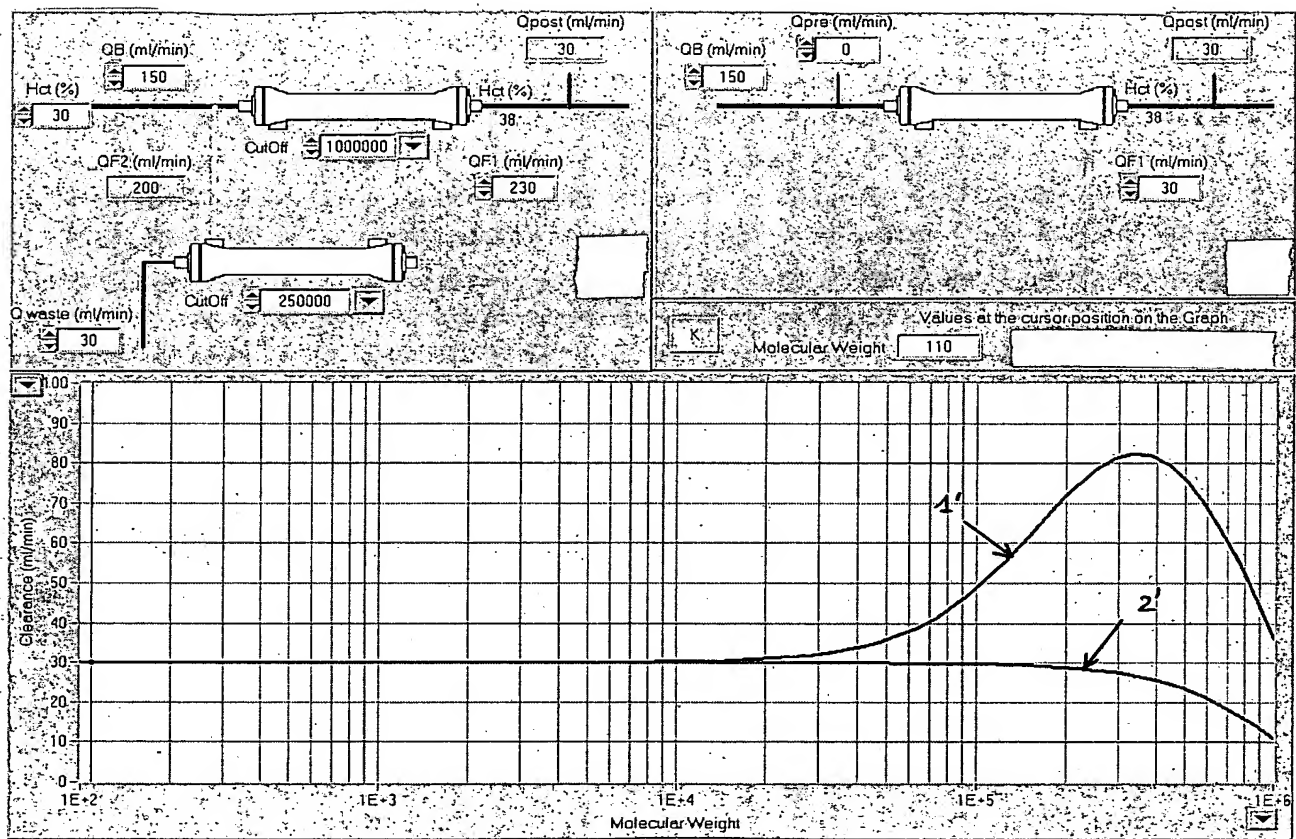


Fig. 12

BEST AVAILABLE COPY